

CHARITY HOSPITAL  
STATE OF LOUISIANA  
NEW ORLEANS

Finger ring

Washer which fits over plunger and screws into ring cap thus fastening it into place.

Spring strip which increases plunger syringe friction by pressing on cap.


Screw cap

Thin brass tubing containing offset pieces containing screw threads for cap + valve piston.

Slider to adjust outward motion of plunger.

Brass tubing to contain four windows to permit visibility of syringe.

7 Parts to assemble

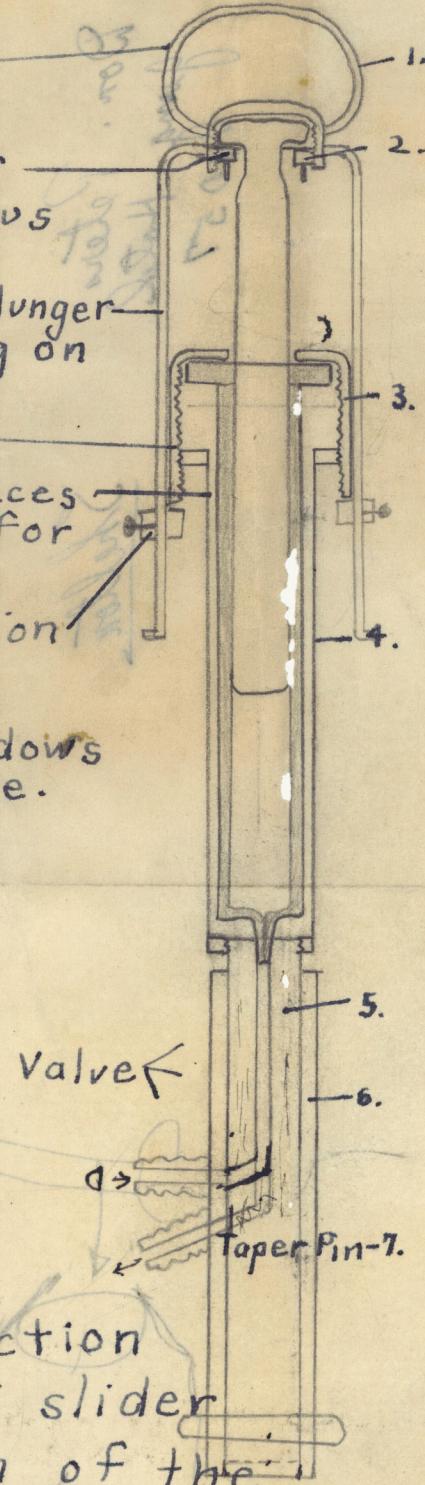


Improvements in the  
Syringe case and friction  
adjusting mechanism + slider  
to limit outward motion of the  
piston.

$6 \times 2 \times 1\frac{1}{2}$

CHARITY HOSPITAL  
STATE OF LOUISIANA  
NEW ORLEANS

Don. Peters  
Jung  
Hotel  
1057

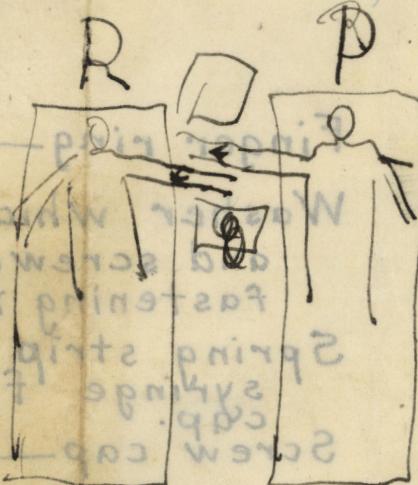


Spindle strip which fits over handle  
fastened to into base.  
Screw base release pressing on  
screw cap.

Shelton  
Slide to adjust outward motion  
of handle.

Base turned to contain four windows  
to permit visibility of shield.

Parts to assemble

Assemble

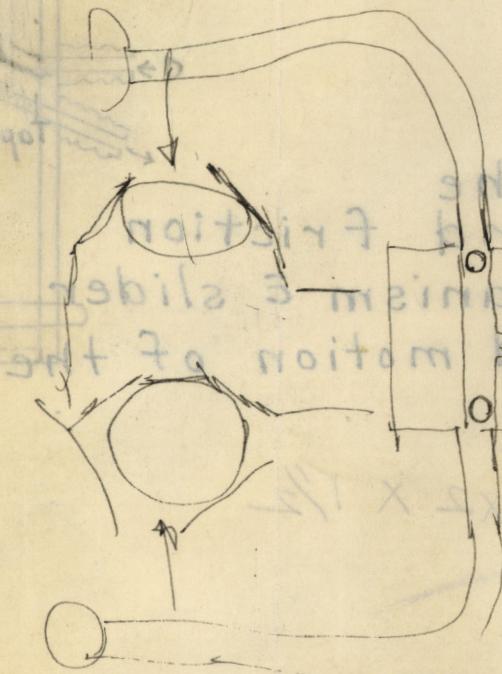

Improvements in this  
shield case are  
adjustable mechanism  
able to limit outward  
motion of pivot.

